



KARIES SCREEN TEST. DE

Check up is good -
testing even better!


Determination of bacterial saliva parameters with KariesScreenTest

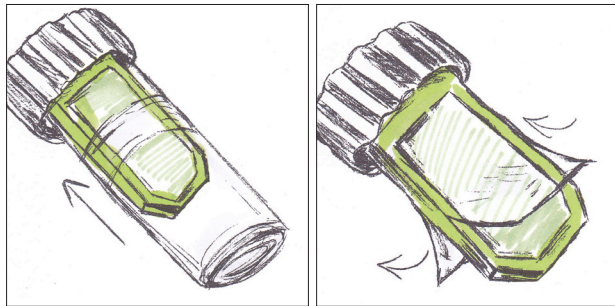

Remove the double dip and pull off
the foil

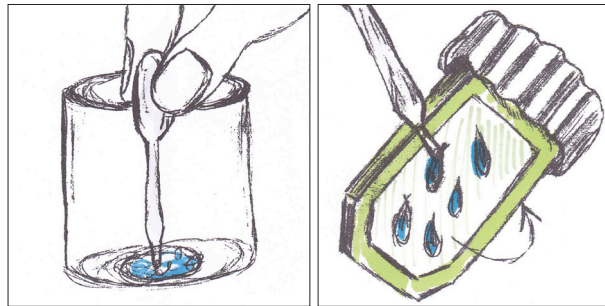


Wet both agars completely with saliva

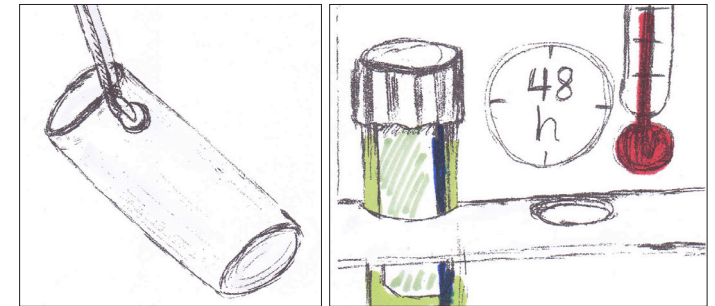


Place NaHCO_3 on the
bottom of the tube

Two days of incubation
time at 37° C

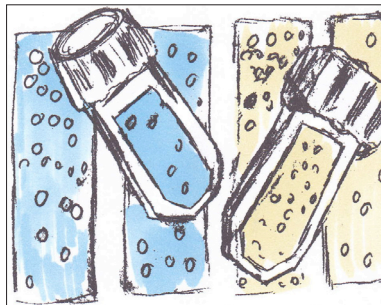


Compare with evaluation chart

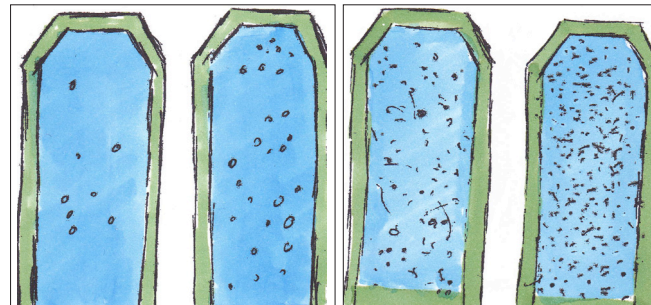

Low colony density

High colony density

Mutans streptococci

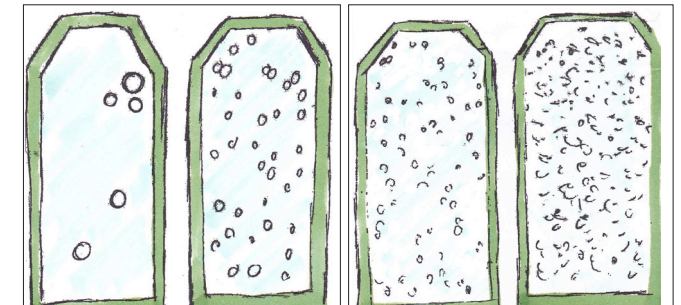

Low colony density

High colony density

Lactobacilli